

NT[®] OPTIMA

CE 1984

ISO 22112 : 2017

ISO 13485 : 2016


TOROSDENTAL İNŞ. İTH. İHR. SAN. VE TİC. A.Ş.
VARSAK MENDERES MAH. 6911 SOKAK NO:3
KEPEZ / ANTALYA / TÜRKİYE

TEL: +90 242 247 76 16 - FAX: +90 242 244 02 14

export@torosdental.com export@teethmanufacturing.com
www.torosdental.com www.teethmanufacturing.com

www.torosdental.com




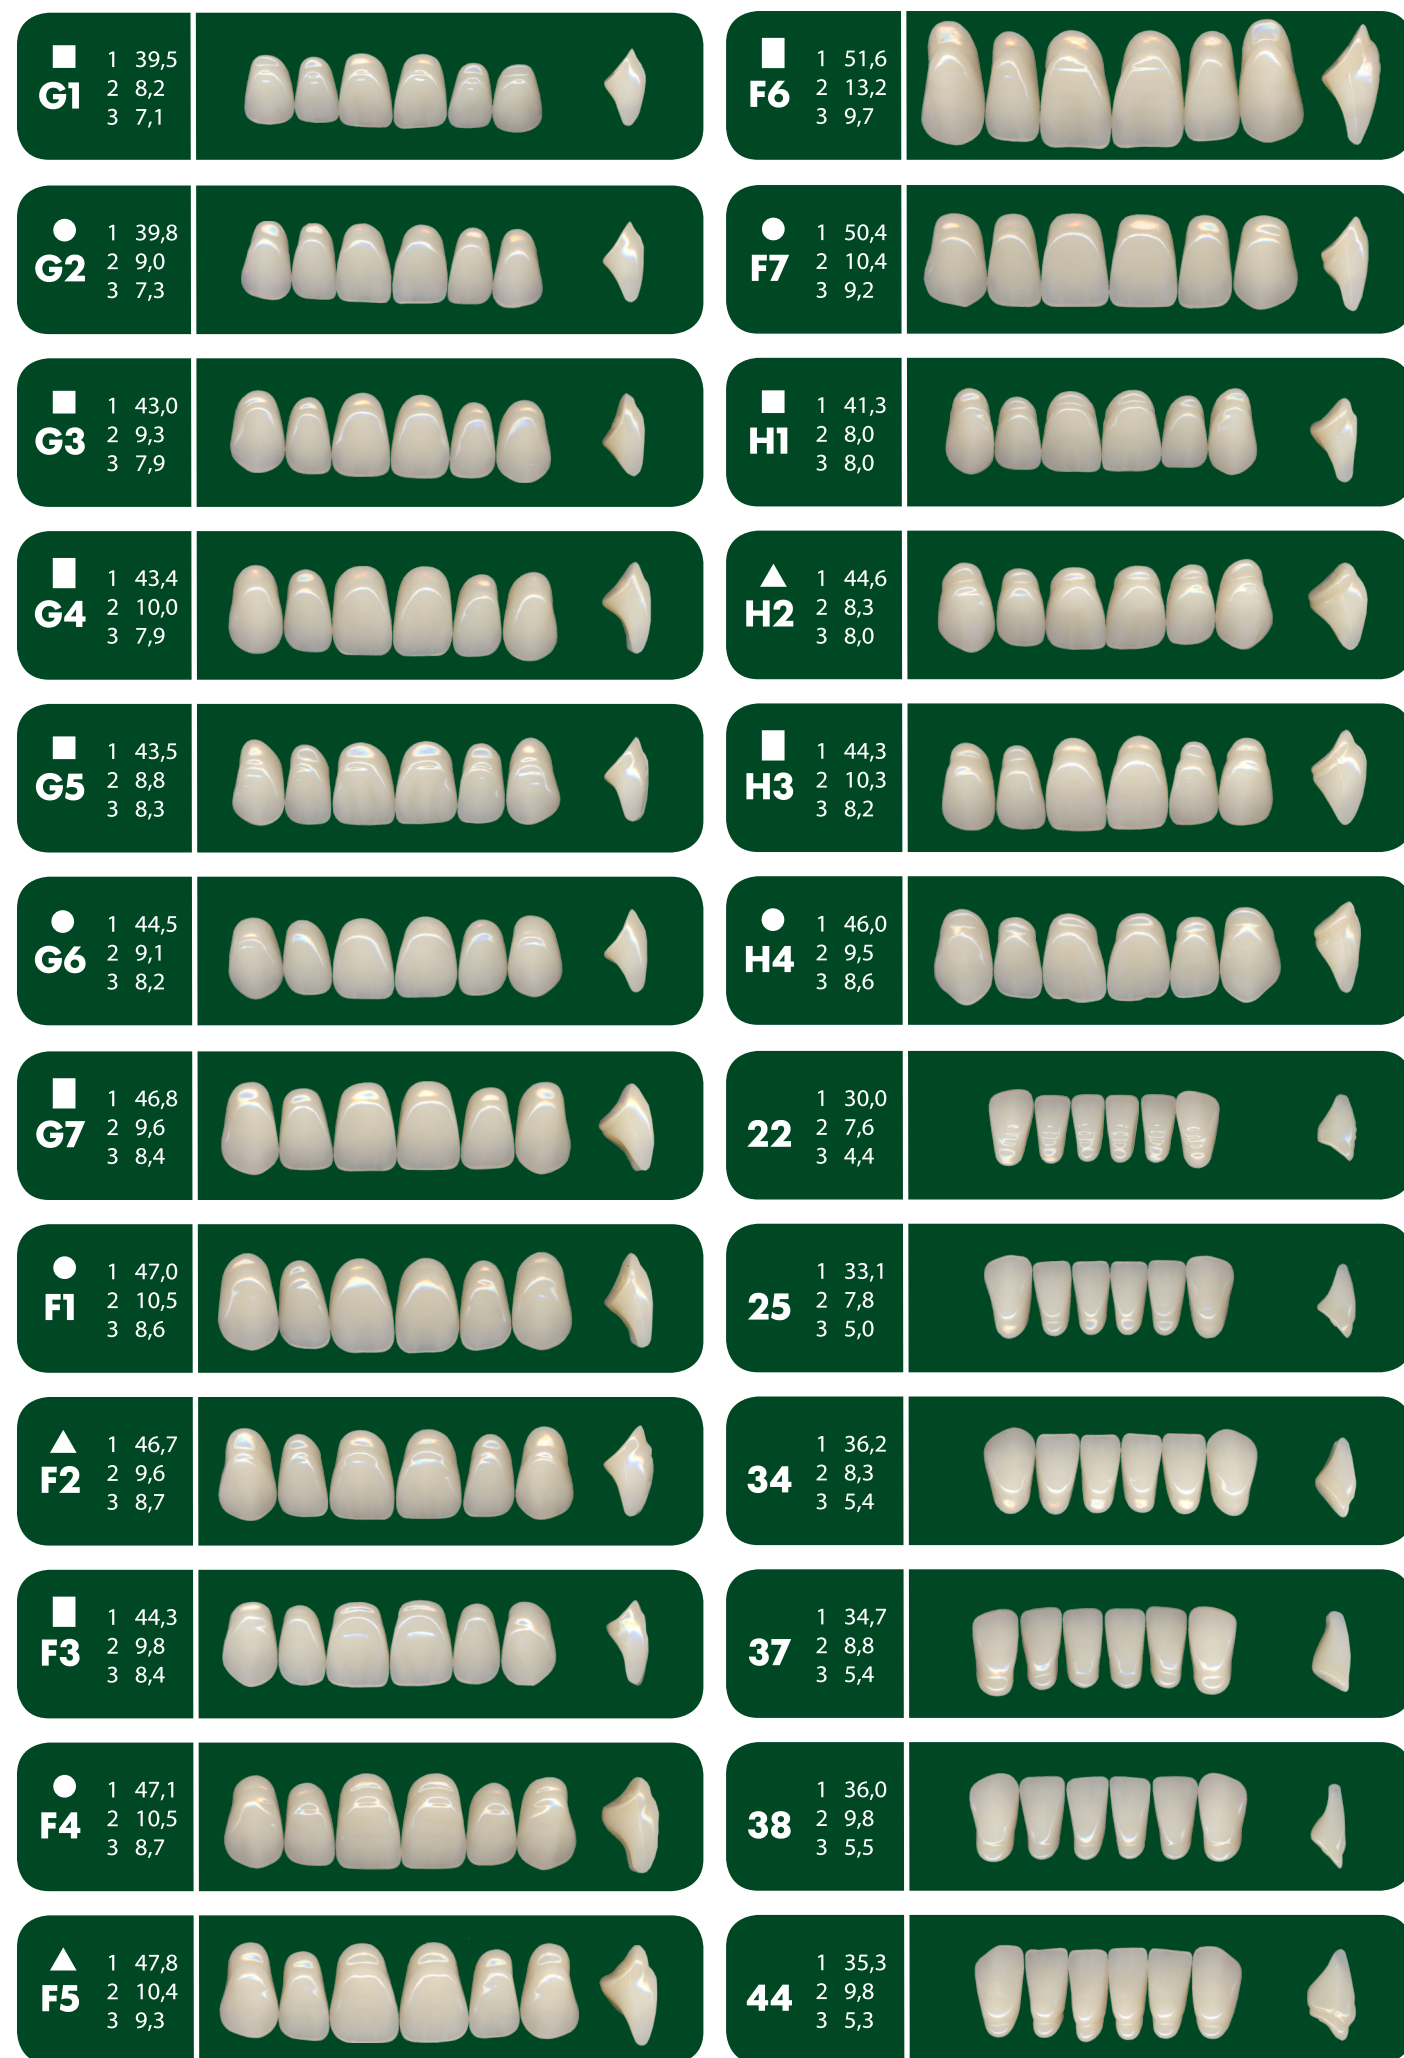


* Ölçülendirme mm olarak verimiştir.



Kombinasyon Çizelgesi Combination Chart

	22	29
G1	22	29
G2	25	31
G3	25-34	31-33
G4	37	33-35
G5	25-34	33
G6	37	35
G7	37	35-39
F1	38	35-39
F2	38	35-39
F3	38	35-39
F4	67	39
F5	74	39-41
F6	88	41
F7	58	41
H1	25	31
H2	34	33
H3	44	35-39
H4	44	35-39

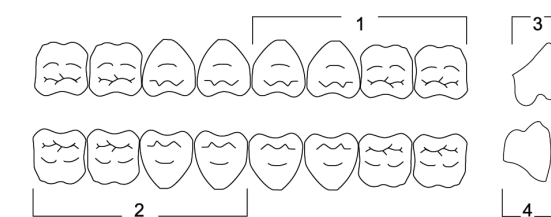

* All measurements given are in mm form



BABY TOOTH